

Simplant Surgical Guide Proposed Plan

Date: X

Patient Name/ID: X



Proposed Implant Site/s: 45, 46

Guided Implant System: ASTRA SAFE GUIDE

Plan for Clinician: X

Approved by _____

Implant information

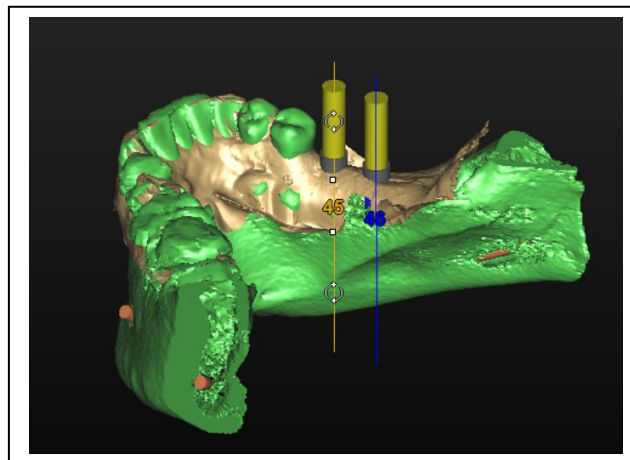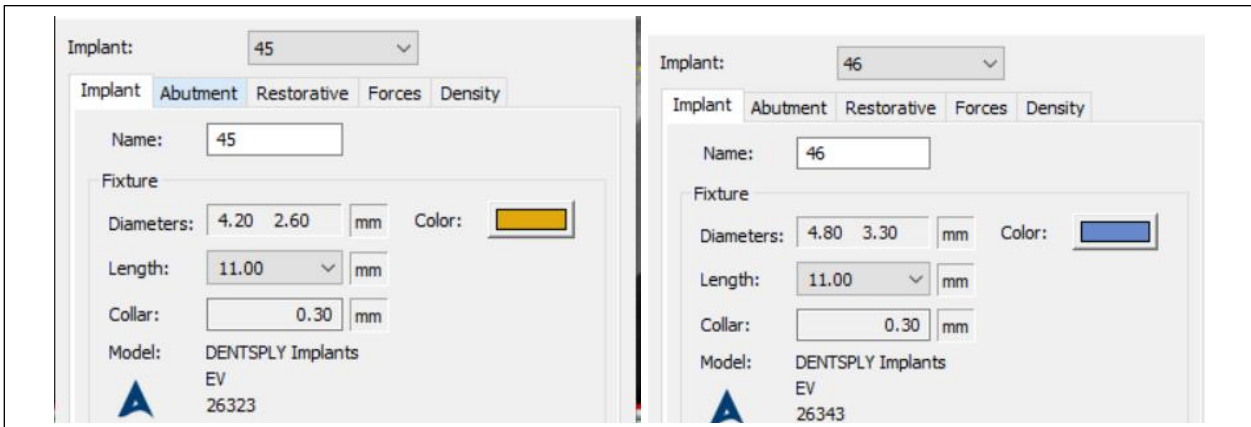


Limitation of Liability


This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.

Implant 45

Cross Sectional view

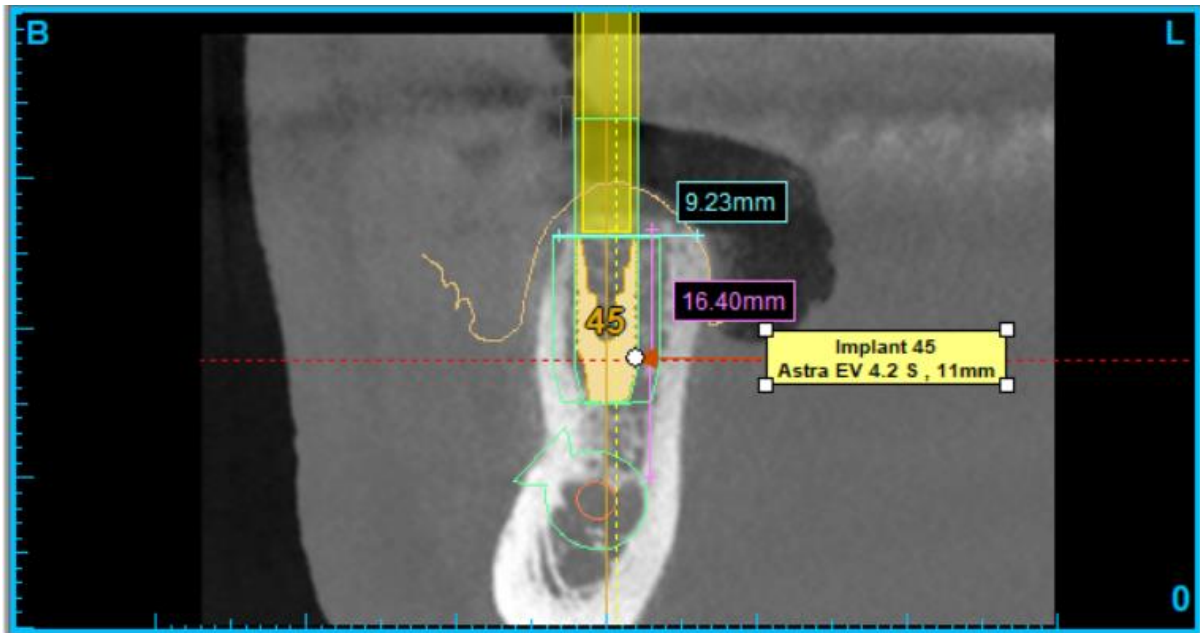


Axial View

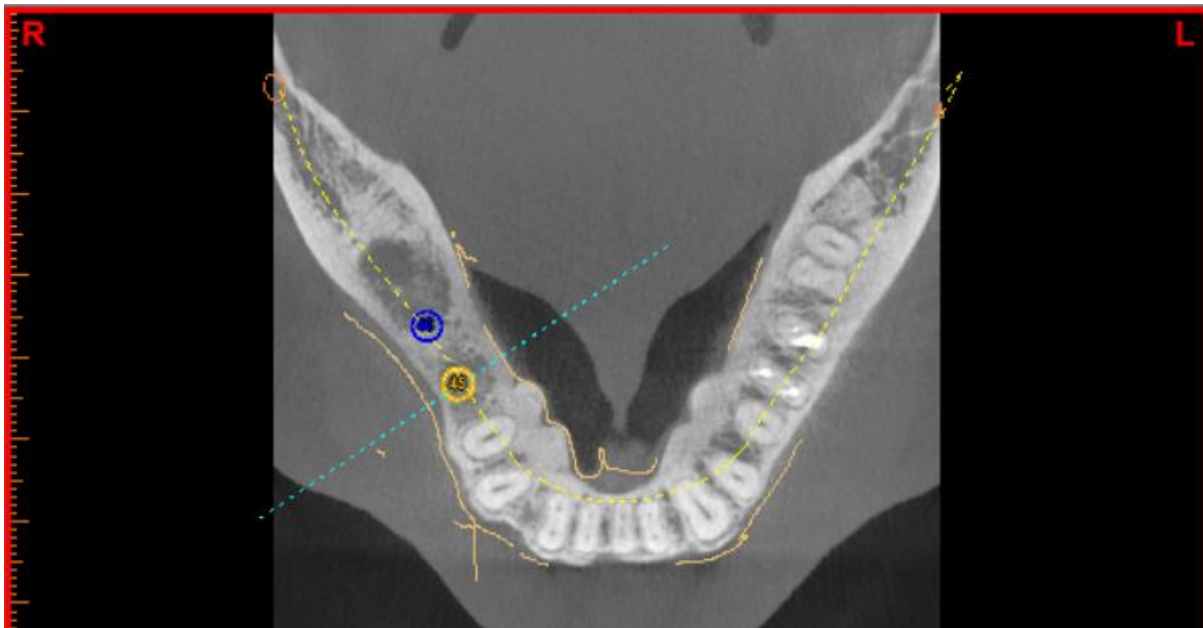

Limitation of Liability


This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.

Panoramic View

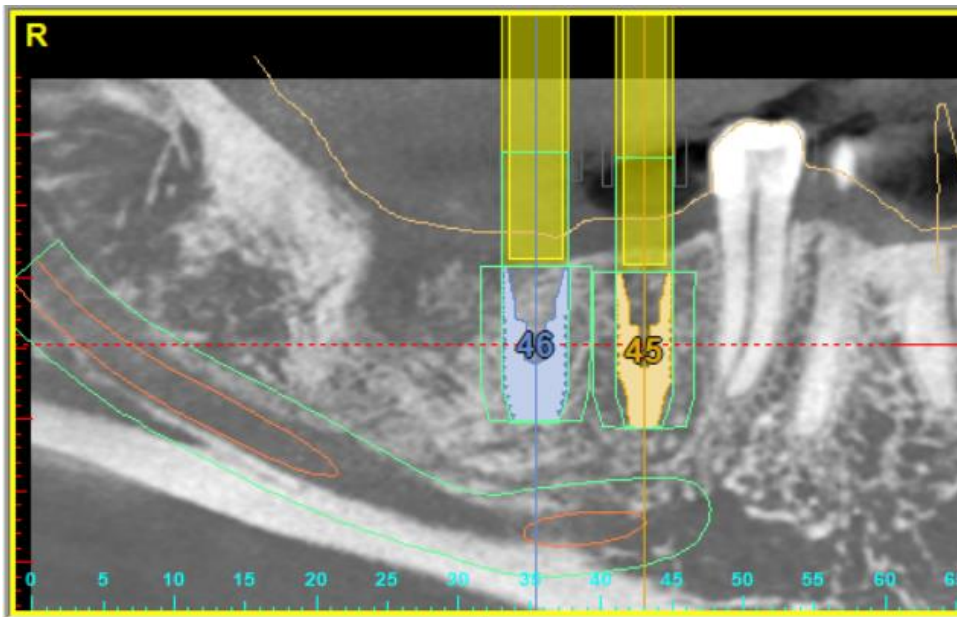

Bone Density Chart

Bone Density Graph

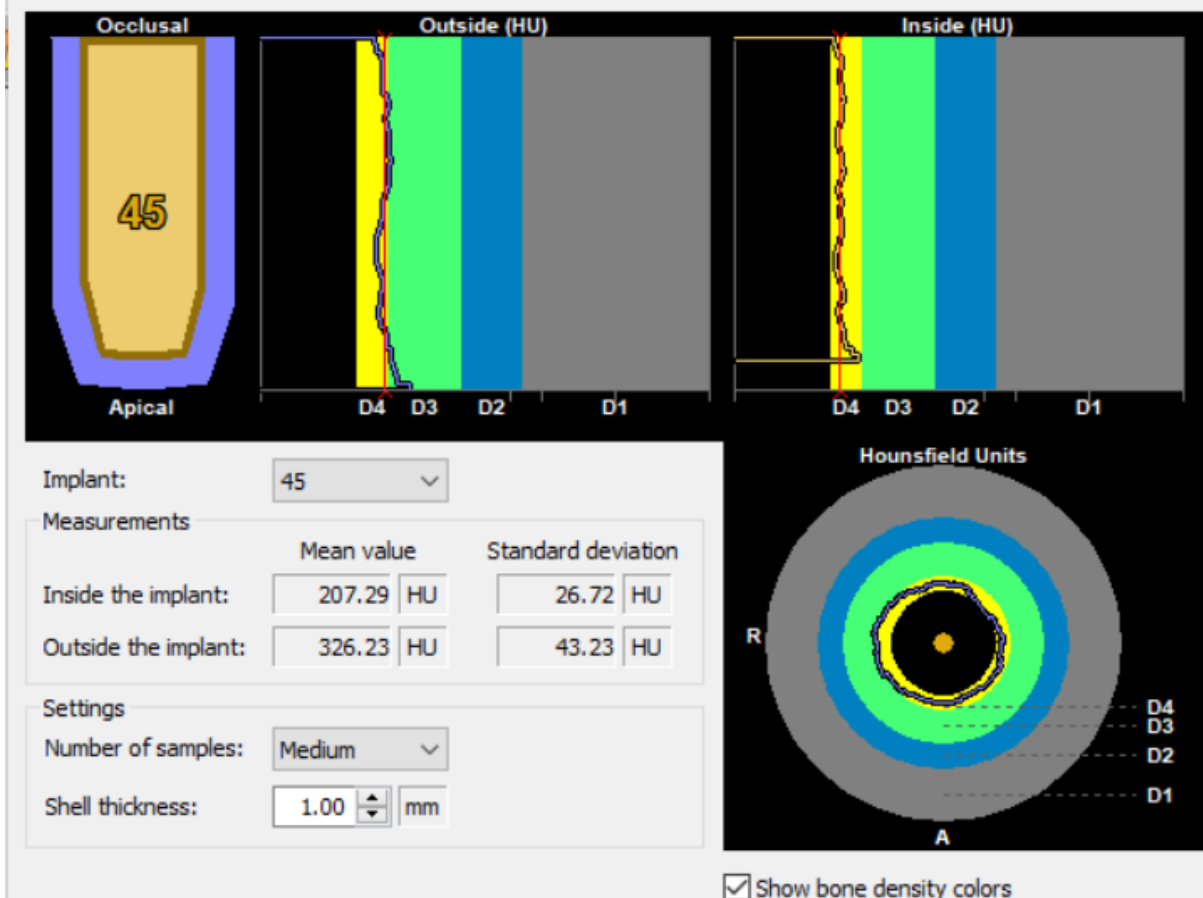


Limitation of Liability


This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.

Implant 46

Cross Sectional View

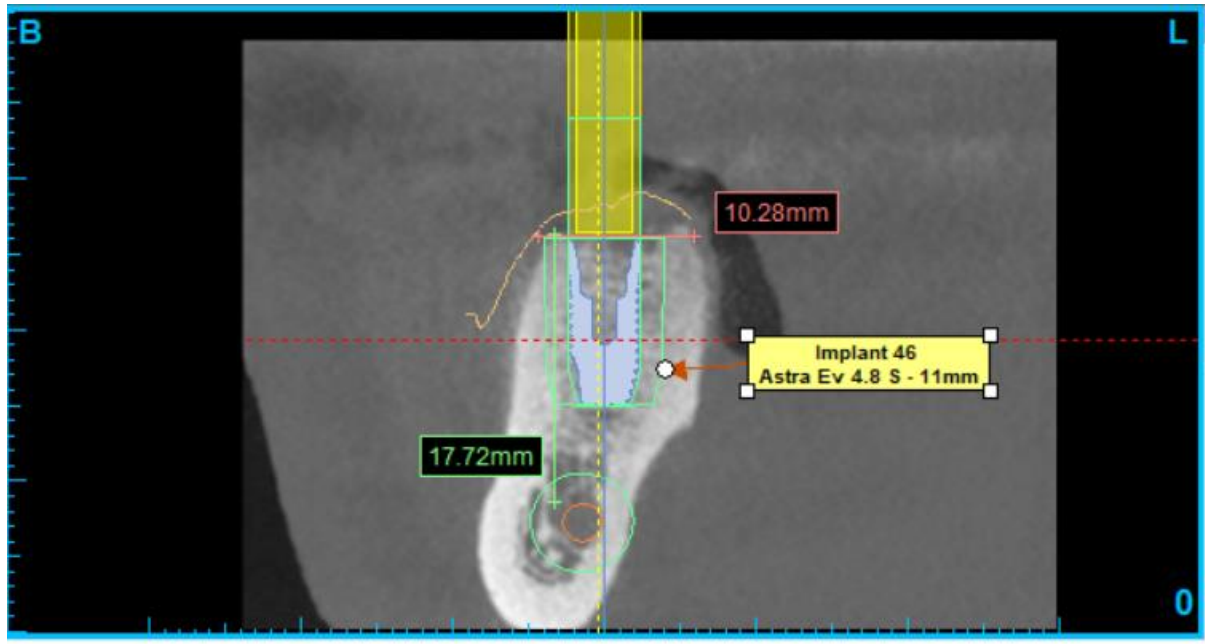


Panoramic View

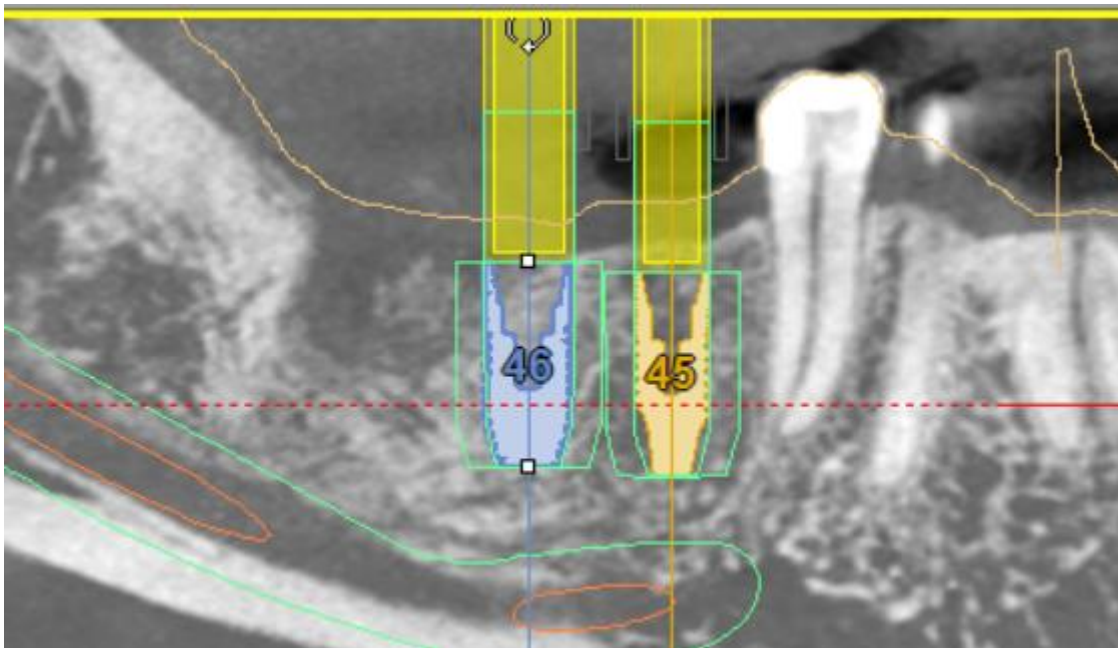


Limitation of Liability

This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.

Axial View

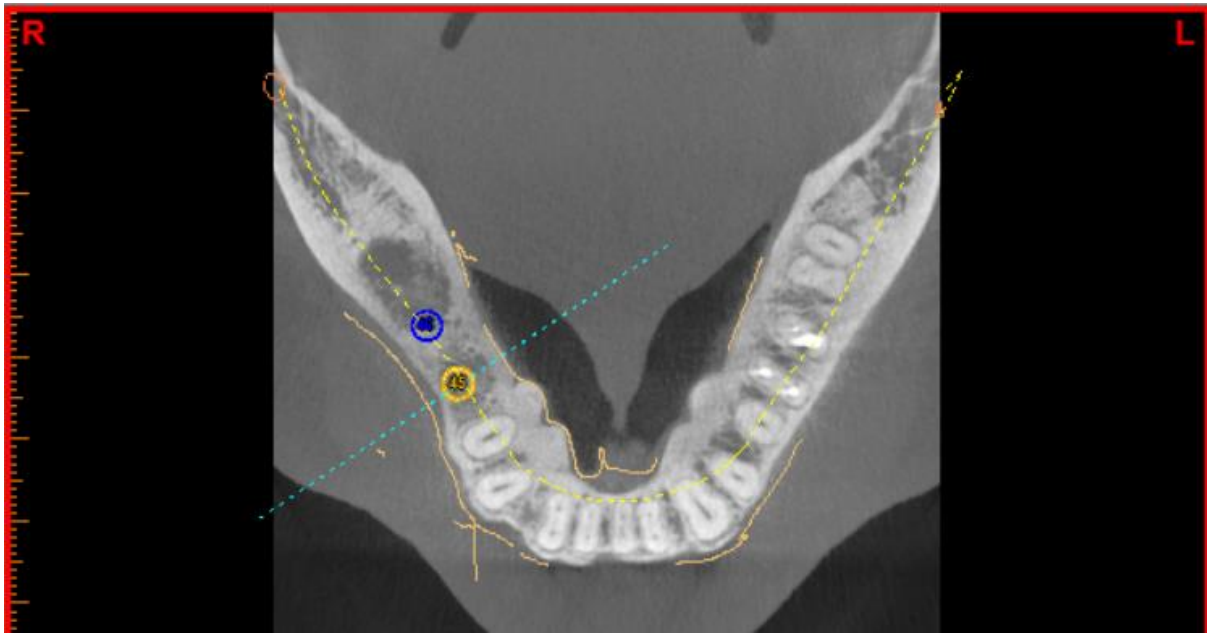

Bone Density Graph

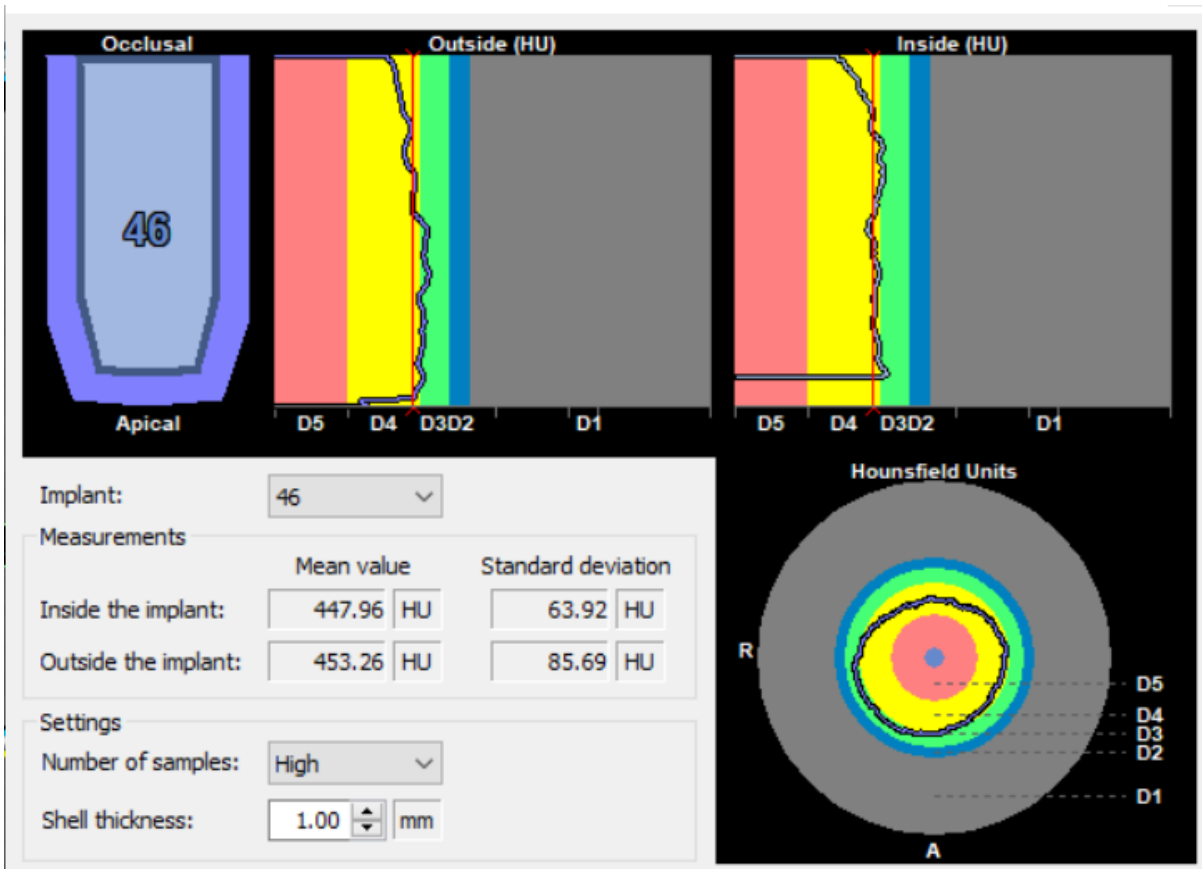


Limitation of Liability

This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.

Implants planned parallel to each other

Angle on the implant level	Angle on the abutment level	Distance between occlusal points
Implant name	To reference implant	To prosthetic insertion axis
<input checked="" type="checkbox"/> 46	0.0°	0.0°
<input type="checkbox"/> 45	0.0°	0.0°

Proposed Simplant Surgical Guide

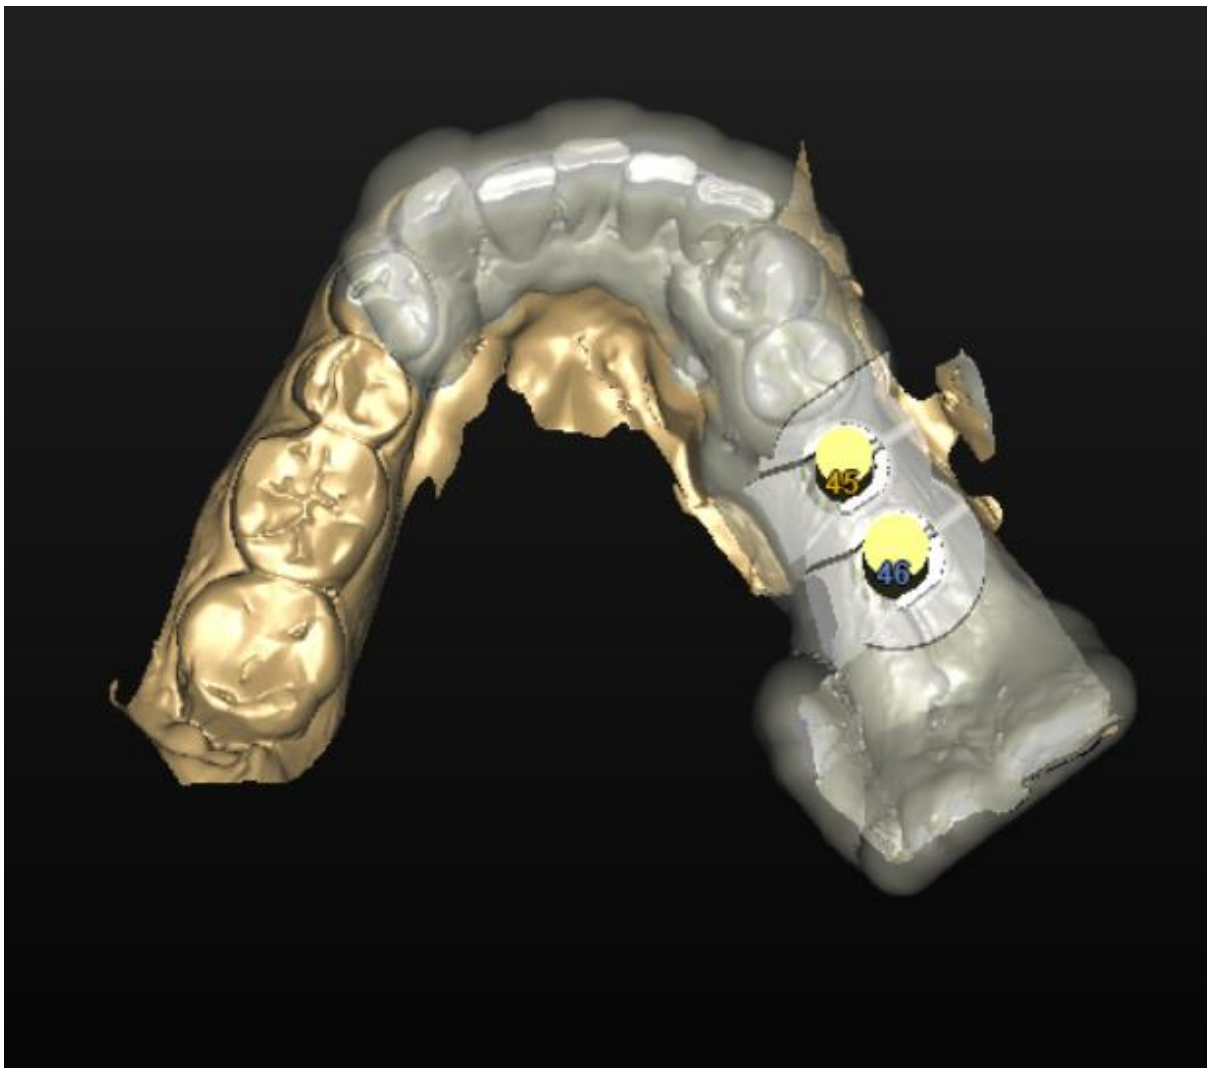





To make any changes to the plan please reply via email otherwise please carefully read the terms and conditions set out below and complete and sign the approved section.

Limitation of Liability

This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.

Implant Summary Page

Implant 45

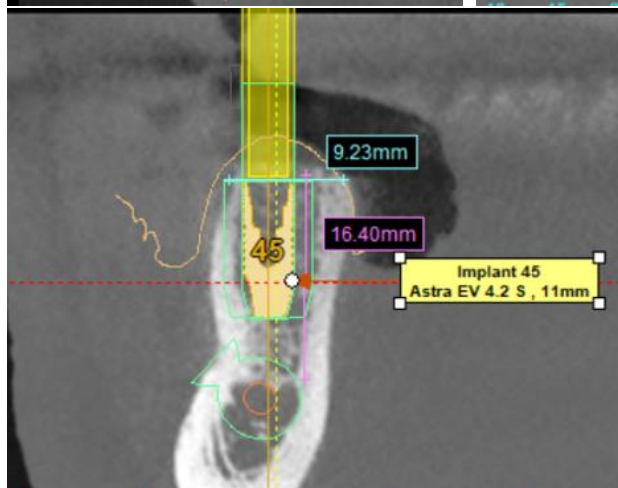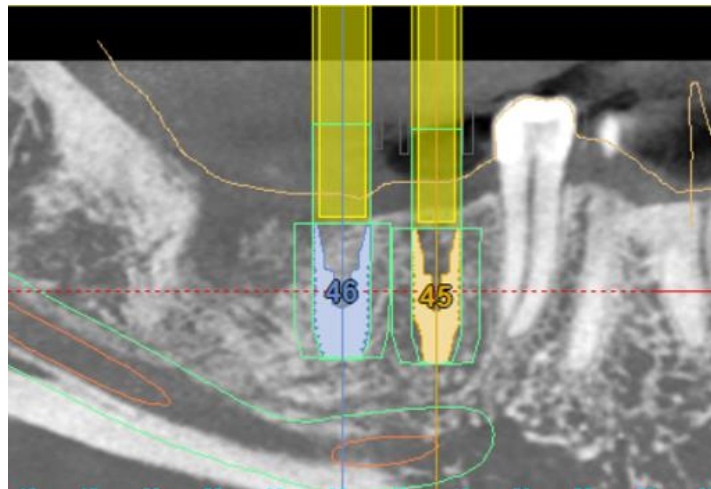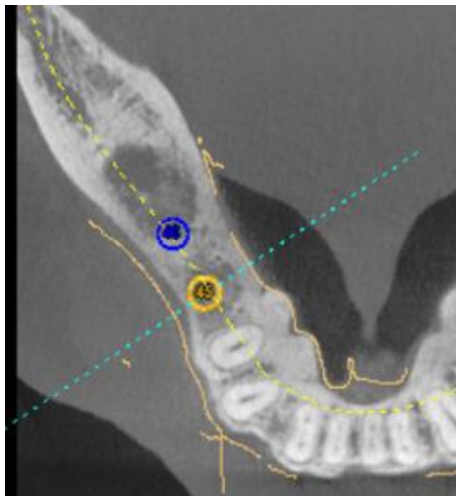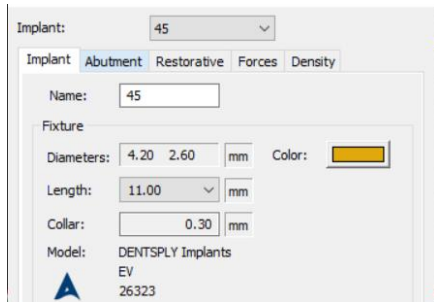

Limitation of Liability

This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.

Implant Summary Page


Implant 46

Implant: 46

Implant Abutment Restorative Forces Density

Name: 46


Fixture

Diameters: 4.80 3.30 mm Color: 

Length: 11.00 mm

Collar: 0.30 mm

Model: DENTSPLY Implants
EV
26343

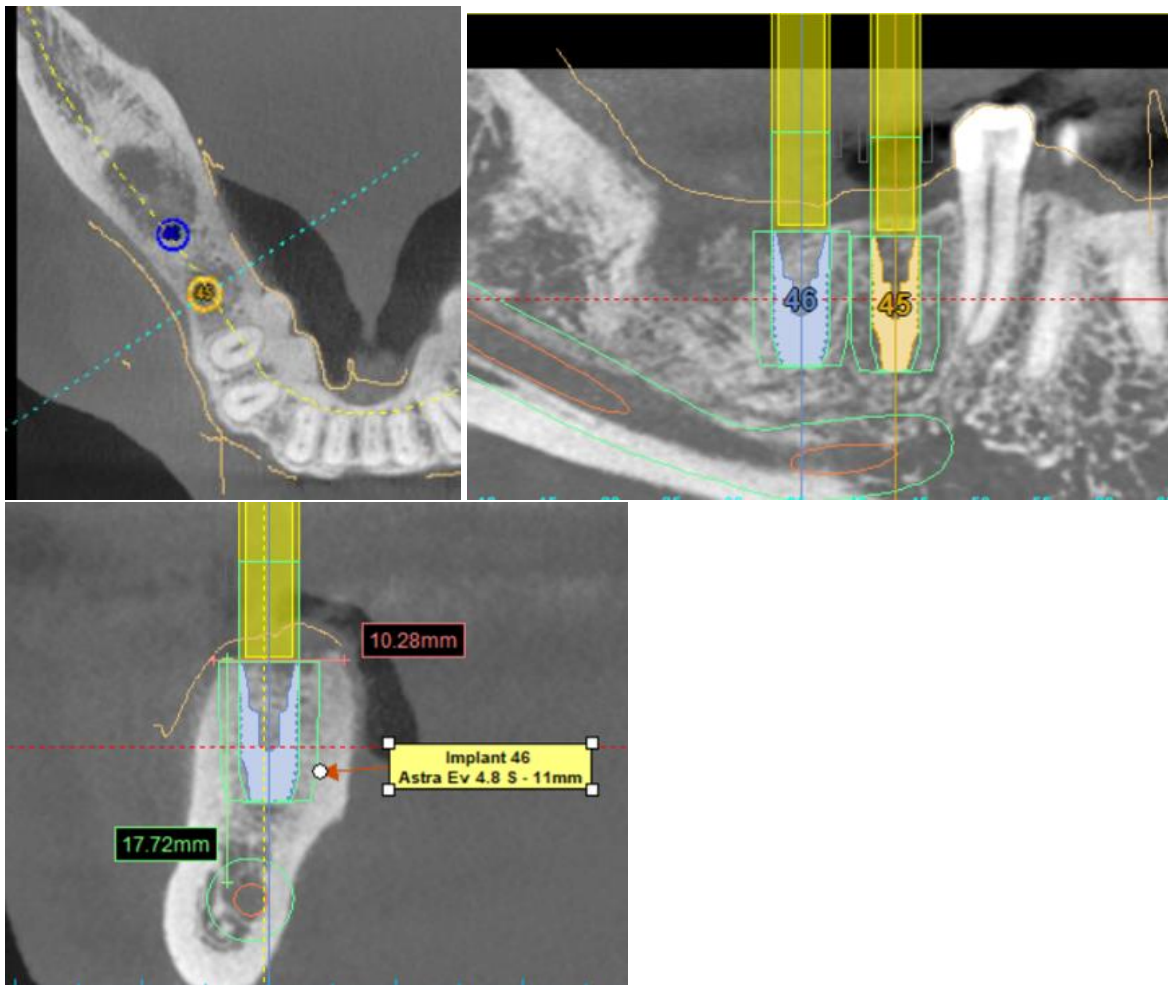

At site 46 Ensure X Drill is used otherwise binding of the implant may be observed prior to full seating of implant in to the ostetomy at proper length.

Limitation of Liability

This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.

Terms and Conditions to Produce Simplant Surgical Guide

Terms and conditions:

The Clinician understands and acknowledges that Premium Dental Lab (PDL) is the supplier of the surgical guide ordered in this document. The circumstance in which this product is ordered and used are only under the control of the Clinician, and the Clinician assumes full responsibility for the case planning and outcome. The Clinician agrees to verify the conformity of any delivered product with their order before using it. Should the Clinician omit to perform such control or decide to use a non-conformable product, PDL is free from any liability for the consequences of the use of such a product. The surgical guide represents only a suggestion for treatment. The Clinician must verify if the surgical plan corresponds to their preoperatively designed surgical plan prior to surgery, and assess the appropriateness of its use clinically. Provision of the surgical guide does not in any way infer or give any Clinician authorisation to use the guide clinically. The Clinician is solely responsible to ensure they have the relevant experience, qualifications and/or licences as required by law to make such a request from PDL, and to use the provided surgical guide clinically. The Clinician is solely responsible for the actual surgery performed, regardless of the virtual planning. Any adjustments in the surgical plan in the event of a variance between the clinical situation and the virtual planning is at the sole discretion of the clinician.

The liability of PDL for real and proven damages, regardless of the gravity of the failure are limited to the price of the product directly related to the claim. Under no circumstances can indemnity be grounded for indirect damages such as, but not limited to: loss of revenue, increases expense, loss of customers or goodwill, loss of benefits or expected savings or any other financial or commercial losses which are not direct and immediate consequences of a shortcoming of PDL in its obligations. PDL is not responsible for any shipping delays outside of it's own control. PDL products must be used in accordance with any instructions for use provided by the manufacturer. PDL makes no warranty, express or implied, except that all PDL products shall be free from defects in material and workmanship. Any warranty applies only to the original buyer and is non transferrable. No amendments or modifications may be made to this document unless in writing and duly executed by and authorised representative of PDL. These terms and conditions are to be read together with Premium Dental Lab Account Terms and Conditions and are governed by the laws of the state of Queensland. The Clinician, by signing this form, understands, acknowledges and agrees to all the "terms and conditions" and requests that a surgical guide be manufactured by PDL in accordance with their approved surgical plan.

Approved by _____

Signed _____

Date _____

Limitation of Liability

This instruction incorporates a custom document that is based on a surgical plan proposed by the surgeon before operation. The surgeon, therefore, takes full medical responsibility for the design and the application of the surgical guide, the intended used surgical tray kit, implants and sleeves – all as specified on the order form received by the supplier. The custom document shall be considered as an addition to all other documents sent with and pertaining to the case, and it does not replace any of those other documents.